#### (12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

## (19) World Intellectual Property Organization

International Bureau



# 

(43) International Publication Date 14 October 2004 (14.10.2004)

#### (10) International Publication Number WO 2004/086984 A1

(51) International Patent Classification7:

A61B 17/11

(21) International Application Number:

PCT/GB2004/001350

(22) International Filing Date: 31 March 2004 (31.03.2004)

(25) Filing Language:

English

(26) Publication Language:

**English** 

(30) Priority Data: 0307826.8

4 April 2003 (04.04.2003)


- (71) Applicant (for all designated States except US): UCL BIOMEDICA PLC [GB/GB]; Finance, University College London, Gower Street, London WC1E 6BT (GB).
- (72) Inventors: and
- (75) Inventors/Applicants (for US only): SWAIN, Christopher, Paul [GB/GB]; 41 Willow Road, London NW3 1TN (GB). MOSSE, Charles, Alexander [GB/GB]; 21 Parliament Hill, London NW3 2TA (GB). FRITSCHER-RAVENS, Annette, Dora, Anna [DE/GB]; Flat 3, 18 Bruton Place, London W1J 6LY (GB).

MILLS, Timothy, Noel [GB/GB]; Flat 4, 45 Newman Street, London W1T 1QF (GB).

- (74) Agent: ELKINGTON AND FIFE LLP; Prospect House, 8 Pembroke Road, Sevenoaks, Kent TN13 1XR (GB).
- (81) Designated States (unless otherwise indicated, for every kind of national protection available): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM,
- (84) Designated States (unless otherwise indicated, for every kind of regional protection available): ARIPO (BW, GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: A DEVICE FOR TRANSFIXING AND JOINING TISSUE

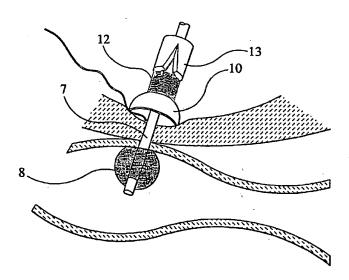

(57) Abstract: A device is provided for use in joining together first and second tissue layers. The device comprises a catheter (7) with an inflatable balloon (8) mounted on the catheter adjacent one end thereof. An inflation channel is provided which is in fluid communication with the interior of the balloon (8) and with a source of inflation fluid, for introducing the inflation fluid into the interior of the balloon (8) is inflated and engages an outwardly facing surface of the first tissue layer and a member, for example a cup (10) or another balloon, engages an outwardly facing surface of the second tissue layer.

## WO 2004/086984 A1



#### Published:

- with international search report
- before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

1

#### A Device for Transfixing and Joining Tissue

This invention relates to methods and devices for transfixing and joining tissues and, more particularly, to forming anastomoses.

In abdominal and vascular surgery anastomosis, the joining together of hollow structures, is an important goal. The ability to establish continuity between two hollow structures can relieve blockage due to cancer, inflammation or other pathology, can allow the removal of abnormal tissue or organs, and, by bypassing a blocked segment, can allow the unimpeded movement of food or facilitate the flow of blood or bile through the body.

Anastomoses are most commonly formed at open abdominal surgery (laparotomy). Hand sewn anastomoses, usually in two or even three layers, are widely performed but are time consuming and require large incisions for hand access. Stapled anastomoses became widely performed especially in colonic surgery since they allowed surgeons to remove low rectal tumours. The short rectal remnant could be joined to the colon above the tumour at a site where it was difficult to place stitches by hand, and in consequence allowed patients to recover without needing a permanent colostomy. The advent of laparoscopic surgery staplers allowed anastomoses to be formed through incisions of 1-2 cm or so that were just large enough to allow passage of these instruments inside the abdominal or thoracic cavity.

Some aids to form anastomoses have been developed. J.B. Murphy, an American surgeon working in Chicago in the 1880's, popularized surgical anastomoses by creating a compression button device for anastomosis. The device had two mushroom-shaped buttons, which could be placed in the two organs to be joined. The buttons could be pressed together by an internal spring in the stalk of the mushroom and the organs would be welded together by the consequent ischaemia (lack of blood supply) at the sites where the buttons were pressed together. Eventually the button device would fall through into the gut, leaving an anastomosis or hole and be passed through the body into the toilet. Compression button anastomoses are still used at open colonic surgery. The use of magnets to compress tissue to form an anastomosis has also been described, and a spring compression button method using a biofragmentable ring has been employed, especially in the rectum.

An anastomosis procedure has been described in an article entitled "Anastomosis as Flexible Endoscopy: an experimental study of compression button gastrojejunoscopy", CP Swain

and T N Mills, Gastrointestinal Endoscopy 1991, 37: 625-631, in which, as its title implies, a method is described of forming anastomoses using a flexible endoscope. The method described there involved introducing a flexible endoscope into one of the two structures to be joined (in this case the stomach), and entering the second of the two structures (in this case the small bowel) by forming an incision in the abdomen of the subject. The present invention is directed, in one aspect thereof, to the formation of anastomoses without the need to make such external incisions, though in other aspects thereof the means described herein which make this possible are applied to anastomoses in the formation of which such incisions are made.

The ability to form anastomoses using flexible endoscopic or percutaneous procedures without opening the abdomen or chest or using laparoscopic methods might offer advantages especially to patients with advanced cancer or in elderly or sick patients, who might withstand conventional surgery poorly. In particular, flexible endoscopy might allow anastomoses to be formed from stomach to small bowel, duodenum to gallbladder, and small bowel to colon.

International patent publication PCT/GB02/02168 describes a number of forms of anastomosis device which can be used, *inter alia*, via an endoscope, and the present application is directed to yet another form of anastomosis device, which can be both simple and effective, and which requires little in the way of novel hardware.

According to the present invention there is provided a device for use in joining together first and second tissue layers, the device comprising a catheter, an inflatable balloon mounted on the catheter adjacent one end thereof, an inflation channel in fluid communication with the interior of the balloon and with a source of inflation fluid, for introducing the inflation fluid into the interior of the balloon, the balloon being adapted, when inflated, to engage an outwardly facing surface of the first tissue layer and a tissue-engaging member adapted to engage an outwardly facing surface of the second tissue layer, whereby the inwardly facing surfaces of the first and second tissue layers are urged into engagement with one another.

In the accompanying drawings:

Figures 1 to 7 show diagrammatically successive stages in the formation of an anastomosis using the device according to the present invention;

Figure 8 shows an alternative pair of anastomosis elements to those shown in the earlier Figures;

Figures 9a to 9d, show embodiments of locking elements for use in the invention; and

Figure 10 shows another alternative type of balloon to that illustrated in Figures 1 to 7. Referring to Figures 1 to 7, an anastomosis is formed as follows between the stomach wall (marked SW) of a patient and the wall of the patient's small bowel (marked SB). It is to be understood, however, that the procedure would be similar if the anastomosis were formed in some other location, for example between the stomach and the gallbladder.

A hollow needle 1 is passed through the biopsy channel 2 of an echoendoscope 3, indicated in the drawings simply by a block. The echoendoscope 3 is provided with means (not shown) for forming an ultrasound image of the region in which the anastomosis is to be formed. A cylindrical tag 4 is slidably received within the hollow needle 1, and the leading end of a thread 5 is attached to the tag 4. The thread passes out of the hollow needle, and thence out through the patient's mouth. The drawing shows the forward end of the needle partially cut away, so that the thread 5, but not tag, can emerge through this cutaway portion. However, it is alternatively possible for this cutaway portion to be omitted, in which case the thread emerges from the forward end of the needle and doubles back over the outside of the forward end on its way to the patient's mouth. As shown in Figure 1, the needle is passed through the stomach wall and its tip passes through the wall of the small bowel.

As shown in Figure 2, the tag 4 is expelled from the end of the hollow needle 1. This is achieved using a pushing rod (not shown) which is passed through the hollow needle behind the tag, and is then withdrawn once the tag has been expelled from the needle. Following expulsion of the tag from the hollow needle, a guide wire 6 is passed through the hollow needle, so that its leading end emerges into the small bowel.

The needle is then withdrawn, leaving the guide wire passing through the wall of the stomach and into the small bowel. Then, as shown in Figure 3, a catheter 7, with a low profile balloon 8 surrounding a portion of the catheter adjacent its tip, is passed over the guide wire, and down through the biopsy channel 2, so that the balloon-carrying part of the catheter 7 passes through the wall of the stomach and into the small bowel. During passage of the catheter through the stomach wall and into the small bowel, a tension is applied to the thread 5 by the person performing the anastomosis procedure, so that the tag 4 pulls the wall of the small bowel into firm contact with the stomach wall in the region through which the catheter 7 is to pass. Although the tag 4 may not always be essential, it is at least helpful in ensuring easier passage of the catheter to the position shown in Figure 3.

As is conventional with balloon catheters, an inflation channel runs within it, separate from the channel through which the guide wire passes, and it is through the inflation channel that a fluid is passed into the balloon 8 to cause inflation thereof. Figure 4 of the drawings shows the balloon in its inflated state.

There are various possibilities are regards the fluid. The fluid could be a gas, for example air, but preferably it is a liquid, since it is easier to avoid leakage with a liquid. Where a liquid is used this could be water, saline, or some other physiologically acceptable liquid. There are, however, other possibilities. In particular, a material can be used to inflate the balloon which is in liquid form at the time it is introduced, but which subsequently becomes solid. For example, an epoxy resin might be introduced into balloon to inflate it, and then left for some minutes to solidify, or it might be possible to solidify the resin by subsequent introduction of a hardener. Alternatively, the material introduced, which might again be an epoxy resin, could be hardened by the use of heat. Such heat could be applied to the liquid in various ways, including:

- (i) Providing the device with an optical fiber which extends from a light source exterior of the patient, through the catheter 7, to the interior of the balloon, where the tip of the optical fiber is blackened so that the line reaching it is converted to heat.
- (ii) If the liquid that is to be hardened is electrically conductive, it could be heated by locating in the interior of the balloon a bipolar electrode, the individual electrodes of which are spaced apart by a short distance, e.g. 2mm, the electrode being connected to an external source of electrical power via electrical conductors which run through the catheter 7.
- (iii) As in (ii) but replacing the bipolar electrode with a diode, resistor, thermistor or other dissipative electrical component.
- (iv) Running a coaxial cable from an external microwave source through the catheter 7 into the interior of the balloon, the frequency of the microwaves being chosen to be such as to cause heating of the particular liquid within the balloon.

Alternatively, a liquid might be used which could be hardened by the application of light.

5

Examples of suitable materials are disclosed in WO 01/50974, to which attention is directed. The light could be introduced into the liquid through an optical fibre arranged as in (i) above, but with the blackened tip omitted.

Once the balloon is inflated it is pulled back, by pulling on the balloon catheter, so as to press the stomach wall and the small bowel wall together very firmly. This is as shown in Figure 5, which also shows an element 11 fixed to the exterior of the catheter. The purpose of the element 11 is referred to in more detail below.

A cup-shaped compression device 10, which can be seen in Figure 6, is then passed down over the catheter 7 and over the element 11, which is an inner locking element. The compression device is in the form of approximately a hemisphere, with an aperture therein of a size larger than the external diameter of the inner locking element 11. This is followed by a compression spring 12 and an outer locking element 13. The elements 10, 12, and 13 are pushed down the catheter 7 by the leading end of an endoscope 14, along whose biopsy channel 15 the catheter 7 passes. For this purpose, the external diameter of the outer locking element 13 must be larger in diameter than the biopsy channel 15.

The endoscope could be the same as the endoscope 3 referred to above, or it could be different. In the drawings, two different endoscopes are shown, which have different view systems at their forward ends. Although this has an advantage in that the best view system for the first part of the procedure may not be the best for the latter part of the procedure, it is of course simpler to use the same endoscope throughout. If that is done it may further be advantageous not to have to withdraw the endoscope after the first part of the procedure and reinsert it for the latter part, something which is necessary when practising the embodiment shown in Figures 1 to 7 and 9, because the compression device 10 and the locking element 13 are too large to pass through the biopsy channel 15. To avoid this problem the compression device can be made in the form of an umbrella, which can be folded in order to pass it through the biopsy channel and then unfolded for use as a compression device. Further, the locking element 13 can be made smaller, so that it will pass through the biopsy channel, and then the locking element 13 can be pushed into engagement with the locking element 11 (described below), not by the end of the endoscope but by an auxiliary pushing catheter which can be passed down the biopsy channel over the catheter 7.

By exerting force on the outer locking element 13, by means of the leading end of the

6

endoscope 14, the cup-shaped compression element is caused to compress the tissue which it engages, so that it becomes one element of an anastomosis-forming device, the other element being constituted by the balloon 8. The spring 12 is forced into compression, and the outer locking element 13 is a snap fit on the inner locking element 11. It may sometimes be possible to omit the spring 12 where the balloon is inflated with gas or a liquid which does not solidify and this can function, at least to some extent, as a spring.

Embodiments of the locking elements 11 and 13 are shown in Figures 9a to 9d. Figure 9b shows the locking element 13 in its rest position, where it can be seen to comprise two legs 20a and 20b separated by a slit and terminating in ratchet teeth 22a and 22b. The locking element 13 is made of a material, for example a plastics material, which is sufficiently resilient to allow the locking element 12 to force the legs apart, as shown in Figure 9c, to allow the locking element to pass beyond the ratchet teeth. Once the locking element has passed beyond those teeth they spring back and prevent the locking element 11 being withdrawn past them. If desired, a plurality of locking elements 11 can be provided along part of the length of the exterior of the catheter 7, so that the locking element 13 can be held in different positions, depending on the thickness of the tissue layers to be compressed, and the extent to which it is desired to compress those layers. The plurality of locking elements can be integrated into a single component, as indicated in Figure 9d by reference 11'.

If the liquid in the balloon is one which does not solidify, e.g. water, the catheter is then sealed, so that the balloon cannot deflate. There are various ways of sealing the liquid inside the balloon. One way of providing sealing is for there to be a one-way valve upstream of the balloon. Another possibility is to fill the catheter lumen with a hot melt, which will seal the water in the balloon when it has cooled and solidified. Yet another possibility is to make a heat seal by simultaneously compressing and heating the catheter, and this could both seal liquid in the balloon and cut the catheter.

When the catheter has not been cut in the course of sealing it, it can be subsequently cut with a guillotine or hot wire in a tube. The situation is then as illustrated in Figure 7. Another possible way of separating the distal part of the catheter 7 from the proximal part is to form a line of weakness in the catheter at the location where separation is required, and then push the two portions apart by pushing on the locking element 13 by means of the distal end of the endoscope or a pushing catheter running through that channel over the catheter 7. Instead of a line of

7

weakness, the catheter 7 can initially be made of two sections joined by a connector, e.g. a sleeve, which holds the two sections together only sufficiently securely to prevent their accidentally separating. The two sections can then be separated in the way just described for the case where a line of weakness is provided.

Although the drawing shows a generally spherical balloon, there are alternative balloon shapes which may be useful. One such shape is a dumbbell, and when a balloon of that shape is used in place of the balloon 8, it may be advantageous for the second anastomosis element also to be a dumbbell-shaped balloon, rather than being cup-shaped, as illustrated in Figures 1 to 7. Figure 8 shows such a pair of dumbbell balloons in the position which they adopt when they are forming the anastomosis, i.e. when the tissue is compressed between them. As shown in Figure 8, there is a first pair of dumbbell-shaped balloons 20, replacing balloon 8, and a second pair of dumbbell-shaped balloons 21, replacing the cup-shaped element 10. It will be seen that these pairs of balloons form an annular region of compressed tissue, which is what is required for an anastomosis to be formed. It will be appreciated that, in use of the arrangement shown in Figure 8, the catheter is initially placed in position and the balloons 20 are then inflated. Once they have been inflated the catheter can be pulled back to cause the inflated balloons 20 to exert pressure on the tissue, and the balloons 21 can then be inflated to press the tissue from the other side.

Yet another possibility is to use a balloon whose shape, when inflated, is as shown in Figure 10, and has a lumen which is larger than the catheter to which it is attached. The aim of using a balloon of this type is to obtain a larger anastomosis than would otherwise be possible. Figure 10 shows a balloon 100 whose shape is that of two interconnected toroids. It surrounds a catheter 101 through which is threaded a guide wire 102. The balloon is shown compressing two layers of tissue 103 and 104. The balloon is inflated via an inflation tube 105, separate from the catheter 101. For the purpose of introducing the balloon, it can be folded on the outside of the catheter and adhered to one side thereof. If the degree of adherence is low, it will separate from the catheter on expansion, and the catheter can then be removed, leaving the balloon in the desired position in relation to the tissue layers. Alternatively, a larger catheter could be slid over the folded balloon, the larger catheter being withdrawn once the balloon has been sealed, or after the liquid in the balloon has become solid, as the case may be.

It is also to be noted that when reference is made herein to the inflatable balloon mounted


on the catheter adjacent one end thereof, it is to be understood that the balloon might be right at the tip of the catheter, even to the extent that the leading end of the balloon is a short distance, say 5 mm, beyond the leading end of the catheter. Alternatively, the catheter might have a balloon-free lead-in section extending, say, 20 mm or even more, beyond the leading end of the balloon.

#### CLAIMS:


- 1. A device for use in joining together first and second tissue layers, the device comprising a catheter, an inflatable balloon mounted on the catheter adjacent one end thereof, an inflation channel in fluid communication with the interior of the balloon and with a source of inflation fluid, for introducing the inflation fluid into the interior of the balloon, the balloon being adapted, when inflated, to engage an outwardly facing surface of the first tissue layer and a tissue-engaging member adapted to engage an outwardly facing surface of the second tissue layer, whereby the inwardly facing surfaces of the first and second tissue layers are urged into engagement with one another.
- 2. A device according to claim 1, wherein the inflation fluid is a gas.
- 3. A device according to claim 1, wherein the inflation fluid is a liquid.
- 4. A device according to claim 3, wherein the said liquid is one which remains in liquid form after introduction into the balloon, the device further comprising an element for sealing the balloon after introduction of the liquid into the balloon.
- 5. A device according to claim 4, wherein the said liquid is selected from the group consisting of water and saline.
- 6. A device according to claim 4, wherein the said liquid is one which is capable of becoming a solid after introduction into the balloon.
- 7. A device according to claim 6, wherein the said liquid is capable of becoming a solid by application thereto of heat, the device further comprising a heating element for applying heat thereto.

- 8. A device according to claim 6, wherein the said liquid is capable of becoming a solid by application of light thereto, the device further comprising an element for applying light thereto.
- 9. A device according to claim 6, wherein the said liquid is a substance which becomes solid on addition of a hardener thereto, the device further comprising a source of hardener.
- 10. A device according to any preceding claim, comprising a locking system for holding the said tissue engaging member in engagement with the outwardly engaging surface of the second tissue layer.
- 11. A device according to claim 10, wherein the locking system comprises a resilient member for resiliently urging the said tissue engaging member into said engagement.
- 12. A device according to claim 10 or 11, wherein the locking system is arranged to provide locking at a plurality of different spacings between the balloon and the said tissue-engaging element.
- 13. A device according to any preceding claim, wherein the said tissue-engaging element is also an inflatable balloon.
- 14. A device according to any one of claims 1 to 12, wherein the said balloon and the said tissue-engaging member are both parts of a single balloon structure.
- 15. A device according to any one of claims 1 to 13, wherein the said inflation channel is defined within the said catheter.
- 16. A device according to claim 14, wherein the said inflation channel is separate from the catheter.
- 17. A method of joining together first and second tissue layers, which comprises passing through the layers the distal end portion of a catheter having a balloon mounted thereon, inflating

the balloon and causing it to engage a surface of first tissue layer, and causing a tissue-engaging member to engage a surface of the second tissue layer, whereby the first and second tissue layers are urged into engagement with one another.

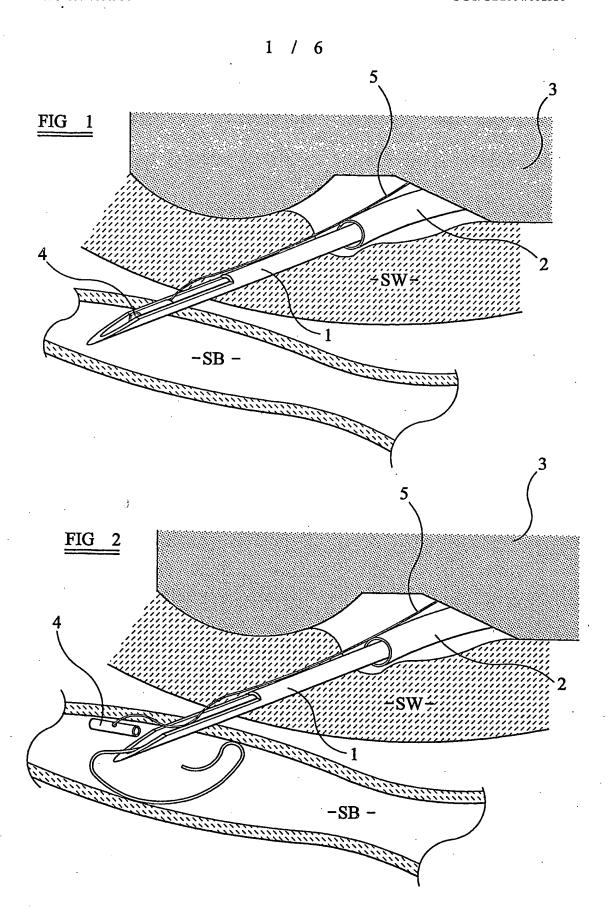


SUBSTITUTE SHEET (RULE 26)

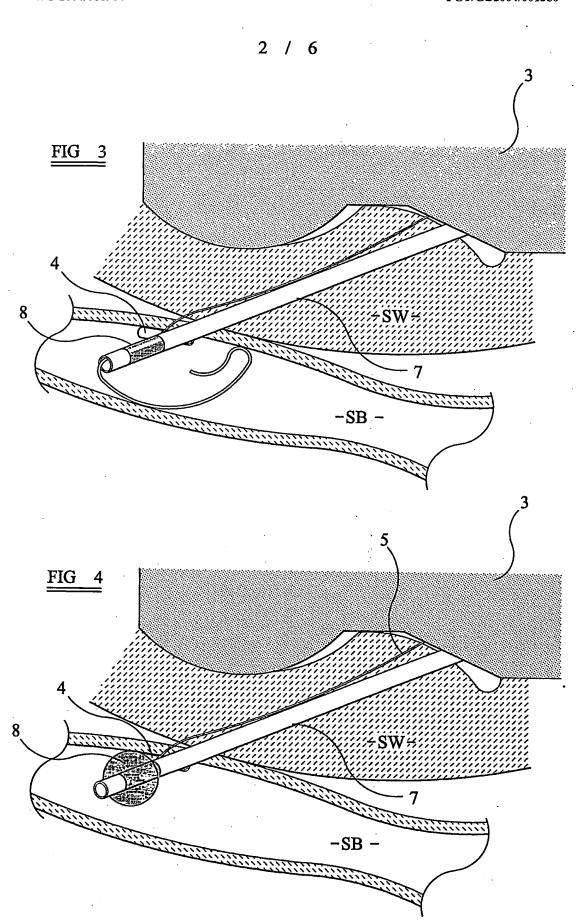



**SUBSTITUTE SHEET (RULE 26)** 


3 / 6

# FIG 5

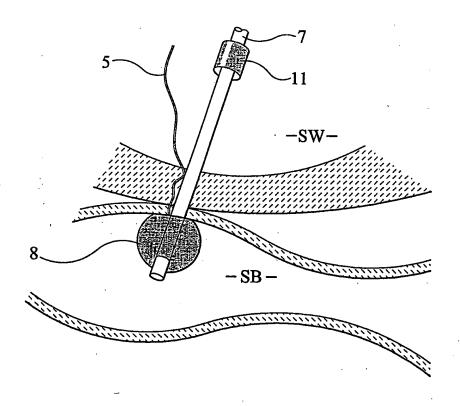


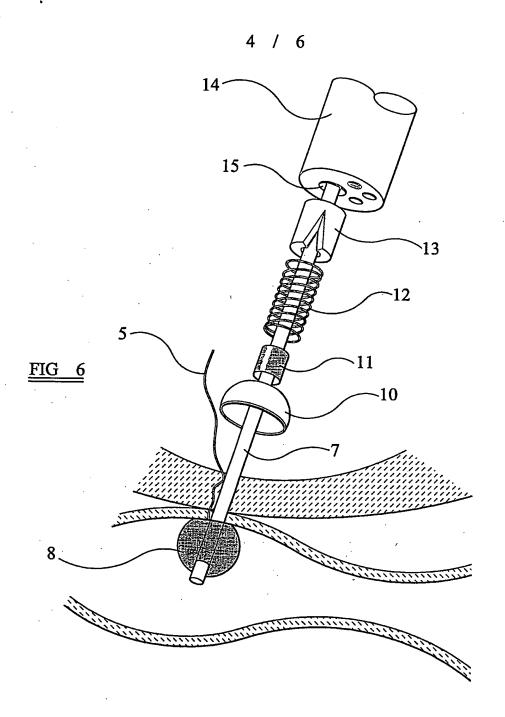


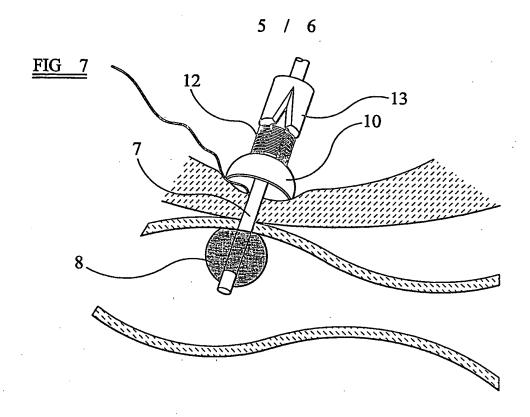


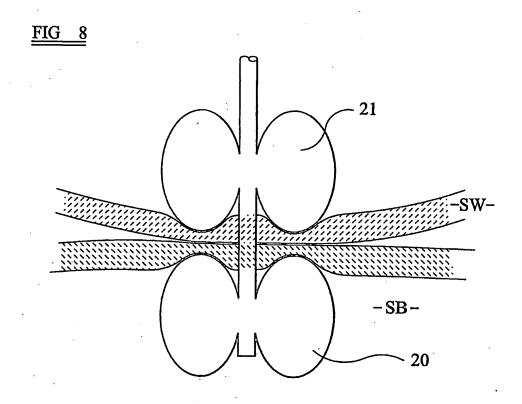

SUBSTITUTE SHEET (RULE 26)

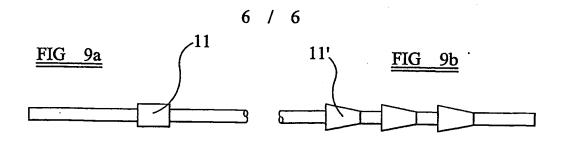

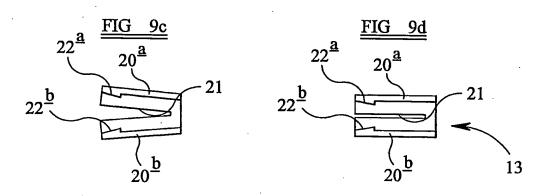

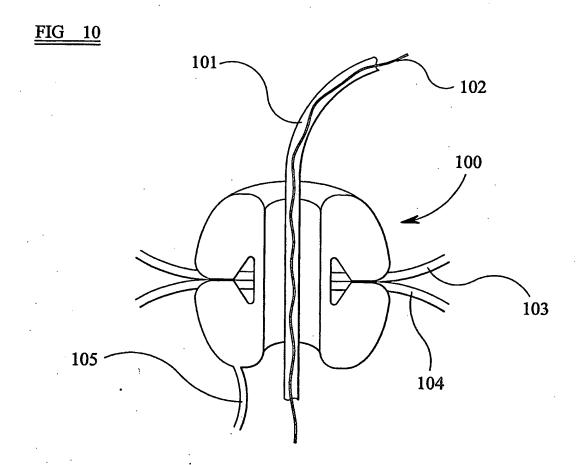

**SUBSTITUTE SHEET (RULE 26)** 

International Application No PCT/GB2004/00135

	_	PCT/GB2	004/001350
A. CLASSII IPC 7	FICATION OF SUBJECT MATTER A61B17/11		
According to	n International Patent Classification (IPC) or to both national classification	ication and IPC	
	SEARCHED		
IPC 7	currentation searched (classification system followed by classification $A61B$	ation symbols)	
Documentat	ion searched other than minimum documentation to the extent tha	t such documents are included in the field	ds searched
Electronic d	ata base consulted during the international search (name of data	pase and, where practical, search terms	used)
EPO-In	ternal	•	
C. DOCUM	ENTS CONSIDERED TO BE RELEVANT		
Category °	Citation of document, with indication, where appropriate, of the	relevant passages	Relevant to claim No.
X	WO 97/13463 A (TRANSVASCULAR INC 17 April 1997 (1997-04-17)	2)	1-9, 13-16
	page 80, line 3 - page 81, line page 82, line 22 - line 29 page 84, line 22 - page 85, line page 85, line 25 - page 86, line figures 8h,9c,9e	e 8	
X	US 5 354 271 A (VODA JAN K) 11 October 1994 (1994-10-11)		1-3, 5-10,12, 14-16
Υ	column 3, line 57 - column 8, l figures 1-7	ine 30	11
	<del></del>	-/	
4	·		
χ Furt	her documents are listed in the continuation of box C.	χ Patent family members are like	sted in annex.
° Special ca	tegories of cited documents:	"T" later document published after the	International filling data
consid	ent defining the general state of the art which is not lered to be of particular relevance document but published on or after the international	or priority date and not in conflict cited to understand the principle invention	with the application but or theory underlying the
"L" docume which	rate ent which may throw doubts on priority claim(s) or is cited to establish the publication date of apother	"X" document of particular relevance; cannot be considered novel or ca involve an inventive step when the "Y" document of particular relevance;	nnot be considered to e document is taken alone
O' docume	n or other special reason (as specified) ent referring to an oral disclosure, use, exhibition or means	cannot be considered to involve a document is combined with one of ments, such combination being of ments.	an inventive step when the or more other such docu-
zater tr	ent published prior to the international filing date but an the priority date claimed	in the art. "&" document member of the same pa	
Date of the	actual completion of the International search	Date of mailing of the International	I search report
4	August 2004	20/08/2004	• .
Name and n	nailing address of the ISA European Patent Office, P.B. 5818 Patentlaan 2	Authorized officer	
	NL – 2280 HV Rijswijk Tel. (+31–70) 340–2040, Tx. 31 651 epo nl, Fax: (+31–70) 340–3016	Nistor, L	

International Application No
PCT/GB2004/001350

- · · · · · · · · · · · · · · · · · · ·		PCT/GB2004/001350			
	ation) DOCUMENTS CONSIDERED TO BE RELEVANT				
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to ctalm No.			
Y	EP 1 262 149 A (KENSEY NASH CORP) 4 December 2002 (2002-12-04)	11			
A	paragraph '0045! - paragraph '0053! figures 9,10,22,23	1			
<b>X</b>	WO 02/066108 A (SHERWOOD SERV AG ; BODICKY RAYMOND O (US); FOURNIE GLENN (US); MEIER K) 29 August 2002 (2002-08-29)	1-10, 14-16			
	the whole document				
Х	US 6 371 974 B1 (CRAGG ANDREW H ET AL) 16 April 2002 (2002-04-16)	1-3,10, 12-16			
	column 5, line 17 - column 7, line 19 column 8, line 1 - line 61 figures 1,4,5				
X	US 3 961 632 A (MOOSSUN MOHAMED H) 8 June 1976 (1976-06-08) column 3, line 13 - column 4, line 23 figure 7	1-3			
A	US 5 304 117 A (WILK PETER J) 19 April 1994 (1994-04-19) column 4, line 17 - line 33 figure 3D	1			
	<del></del>				
	·	·			
		·			

International application No. PCT/GB2004/001350

## INTERNATIONAL SEARCH REPORT

Box II Observations where certain claims were found unsearchable (Continuation of item 2 of first sheet)
This International Search Report has not been established in respect of certain claims under Article 17(2)(a) for the following reasons:
1. X Claims Nos.: 17 because they relate to subject matter not required to be searched by this Authority, namely:
Rule 39.1(iv) PCT - Method for treatment of the human or animal body by surgery
Claims Nos.:     because they relate to parts of the International Application that do not comply with the prescribed requirements to such an extent that no meaningful International Search can be carried out, specifically:
3. Claims Nos.: because they are dependent claims and are not drafted in accordance with the second and third sentences of Rule 6.4(a).
Box III Observations where unity of invention is lacking (Continuation of item 3 of first sheet)
This international Searching Authority found multiple inventions in this international application, as follows:
As all required additional search fees were timely paid by the applicant, this International Search Report covers all searchable claims.
2. As all searchable claims could be searched without effort justifying an additional fee, this Authority did not invite payment of any additional fee.
3. As only some of the required additional search fees were timely paid by the applicant, this International Search Report covers only those claims for which fees were paid, specifically claims Nos.:
4. No required additional search fees were timely paid by the applicant. Consequently, this International Search Report is restricted to the Invention first mentioned in the claims; it is covered by claims Nos.:
Remark on Protest  The additional search fees were accompanied by the applicant's protest.
No protest accompanied the payment of additional search fees.

Form PCT/ISA/210 (continuation of first sheet (2)) (January 2004)

Information on patent family members

International Application No PCT/GB2004/001350

	tent document		Publication		Patent family	Publication
	in search report		date		member(s)	date
WO	9713463	Α	17-04-1997	AU	726713 B2	16-11-2000
				ΑÙ	7431696 A	30-04-1997
				ΑU	729466 B2	01-02-2001
				AU	7595396 A	30-04-1997
				CA	2234361 A1	17-04-1997
				CA	2234389 A1	17-04-1997
				EP	1166721 A2	02-01-2002
				EP	1317908 A2	11-06-2003
				EP	0954248 A1	10-11-1999
				EP	0955933 A1	17-11-1999
				EP	0910298 A1	28-04-1999
				IL	124037 A	12-01-2003
				ΙL	124038 A	19-02-2004
				JP	11513577 T	24-11-1999
				JΡ	11514269 T	07-12-1999
				US	6660024 B1	09-12-2003
				WO	9713471 A1	17-04-1997
	•			WO	9713463 A1	17-04-1997
				US	6068638 A	30-05-2000
				US	6159225 A	12-12-2000
				US	6746464 B1	08-06-2004
				US	6283983 B1	04-09-2001
-				ÜŠ	6231587 B1	15-05-2001
				US	6375615 B1	23-04-2002
				US	2003236542 A1	25-12-2003
				ÜS	2004059280 A1	25-03-2004
				ÜS	6726677 B1	27-04-2004
				US	6655386 B1	02-12-2003
				ÜS	2004133225 A1	08-07-2004
			•	ÜS	2004122318 A1	24-06-2004
			•	ÜS	6190353 B1	20-02-2001
				ÜŠ	6709444 B1	23-03-2004
				ΑŤ	247429 T	15-09-2003
				ΑÜ	733341 B2	10-05-2001
				AU	1847197 A	22-08-1997
				AU	733332 B2	10-05-2001
				AU	1847297 A	22-08-1997
	•			AU	723785 B2	07-09-2000
				AU	1847397 A	22-08-1997
				CA	2244066 A1	07-08-1997
		•		CA	2244079 A1	07-08-1997
			•	CA	2244080 A1	07-08-1997
				CN	1218414 A	02-06-1999
				CN	1216929 A	19-05-1999
				CN	1216930 A	19-05-1999
				DE	69724255 D1	25-09-2003
				DE	69724255 T2	03-06-2004
				EP	0879068 A1	25-11-1998
				EP	0932426 A1	04-08-1999
US	5354271	A	11-10-1994	NONE		
EP	1262149	A	04-12-2002	US	5222974 A	20_06_1002
		n	07 16-200E	US	5282827 A	29-06-1993
				EP		01-02-1994
				EP	1262149 A1	04-12-2002
				EP	0766947 A2	09-04-1997
				AT	0797953 A2 166557 T	01-10-1997 15-06-1998

Information on patent family members

International Application No PCT/GB2004/001350

Patent document cited in search report		Publication date		Patent family member(s)		Publication date
EP 1262149	A		AT	213607	T	15-03-2002
			AU	2121099		13-05-1999
			AU	675777		20-02-1997
		•	AU	3128993		07-06-1993
			AU	5393198		09-04-1998
			AU	704230		15-04-1999
			AU	7178896		23-01-1997
			CA	2122994		13-05-1993
			DE	69225720		02-07-1998
•			DE	69225720		17-12-1998
			DE	69232446		04-04-2002
			DE	69232446		10-10-2002
·			EP	0662802		19-07-1995
			ËS	2117059		01-08-1998
			HK	1011276		28-04-2000
			JP	10305038		17-11-1998
			JP	2904733		14-06-1999
			JP	8173438		09-07-1996
			JP	2506561		12-06-1996
			JP	6510462		24-11-1994
			US	5411520		02-05-199
			US	6045569		04-04-2000
			WO	9308746		
			US	6090130		13-05-1993 18-07-2000
			US	5441517		
			US		A	15-08-199! 28-12-1999
			US	6179863		30-01-200
	-		US	5707393		
			US	5676689		13-01-1998
			US	2001003158		14-10-1997
			US	5861004		07-06-200
			US			19-01-1999
		·		5935147 	A 	10-08-1999
WO 02066108	A	29-08-2002	WO	02066108	A1	29-08-200
US 6371974	B1	16-04-2002	US	6071300	Α	06-06-200
			US	5645566		08-07-1997
			US	2002156495		24-10-2002
			AU	742269	B2	20-12-200
			AU	8293398		08-02-1999
			CA	2295879		21-01-1999
			EP	0994673		26-04-200
			WO	9902091		21-01-1999
i			CA	2231560		20-03-199
	•		ĔΡ	0852478		15-07-199
			ĴΡ	2000507838		27-06-200
			WO	9709934		20-03-199
US 3961632	A	08-06-1976	US	4077412	A	07-03-1978
US 5304117	Α	19-04-1994	NONE		<del></del>	·